


FIG. 1

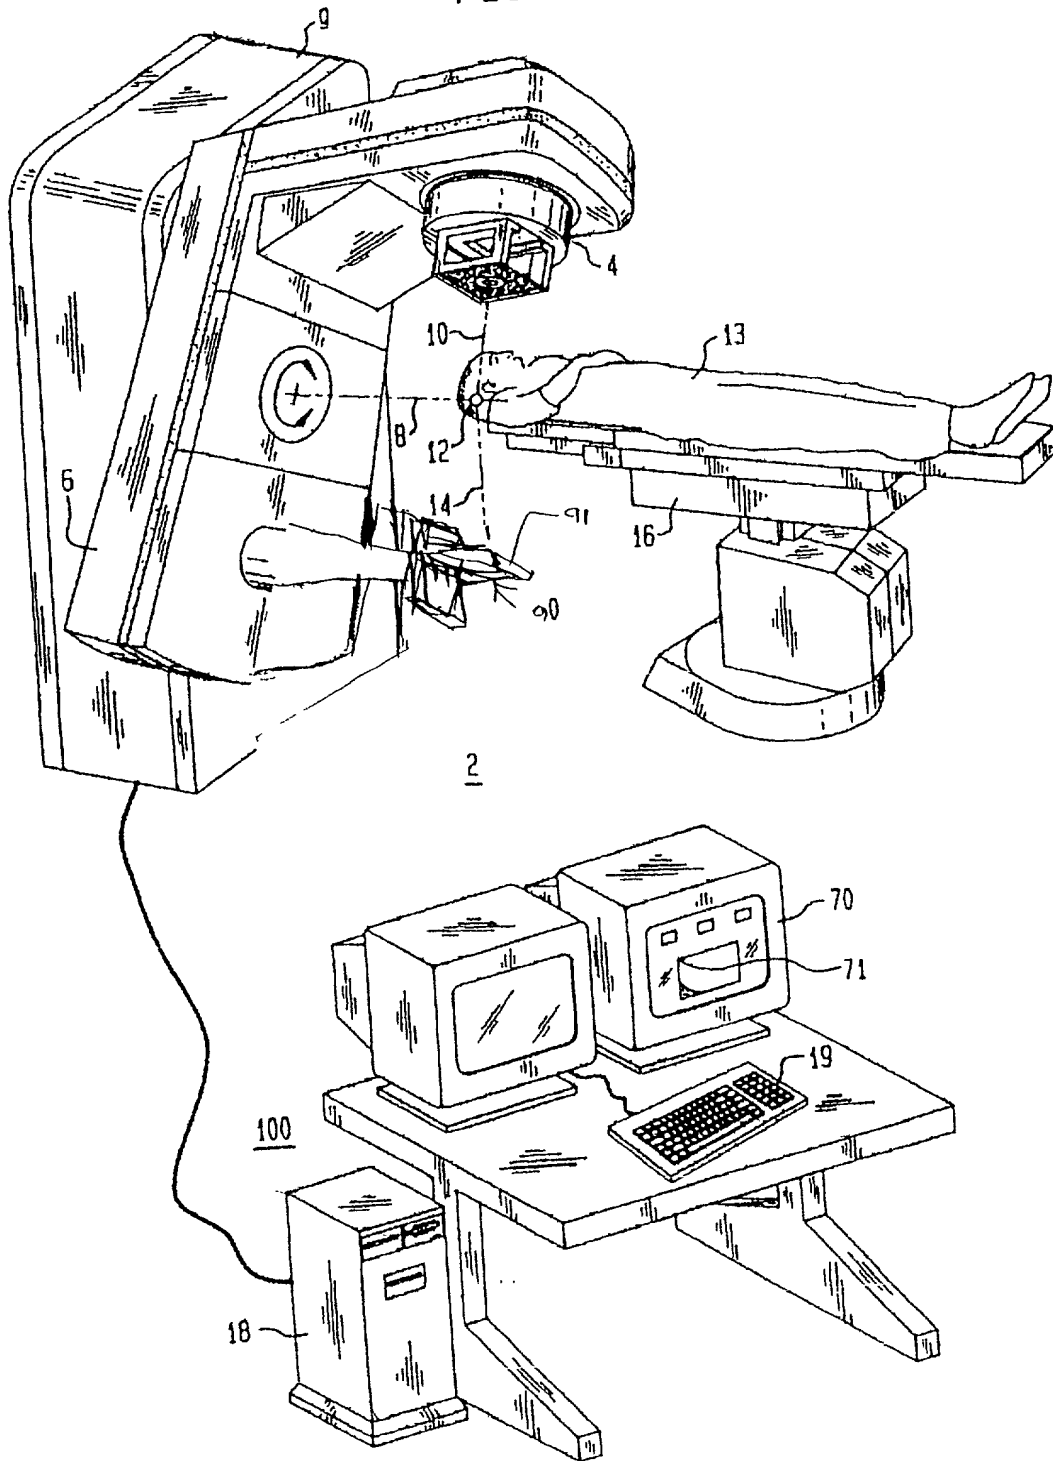


Side view of the patient support assembly 100. The diagram shows the vertical column 102, the base 104, and the patient support structure 106. The horizontal distance from the base to the patient support is labeled as 3088 mm (121.5 in.). The vertical distance from the base to the patient support is labeled as 2576 mm (101.4 in.). The beam axis is indicated by a dashed line and an arrow. The patient plane is indicated by a dashed line and an arrow. The distance from the beam axis to the patient plane is labeled as 252. The distance from the patient plane to the base is labeled as 8a.

Page 2

61

FIG. 3B

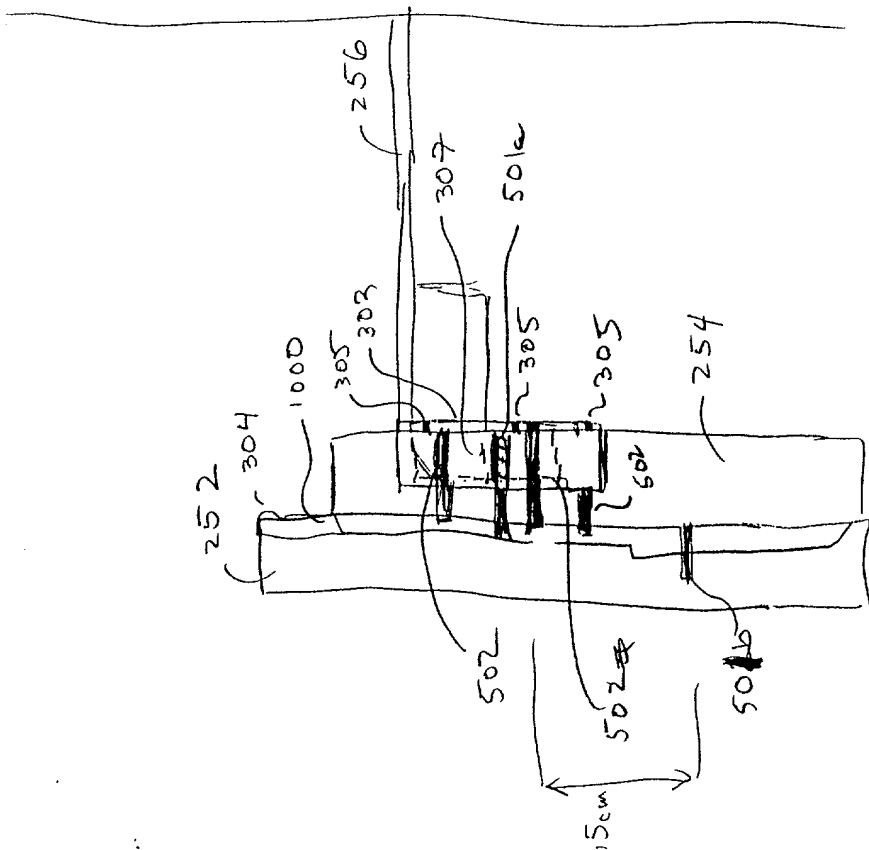

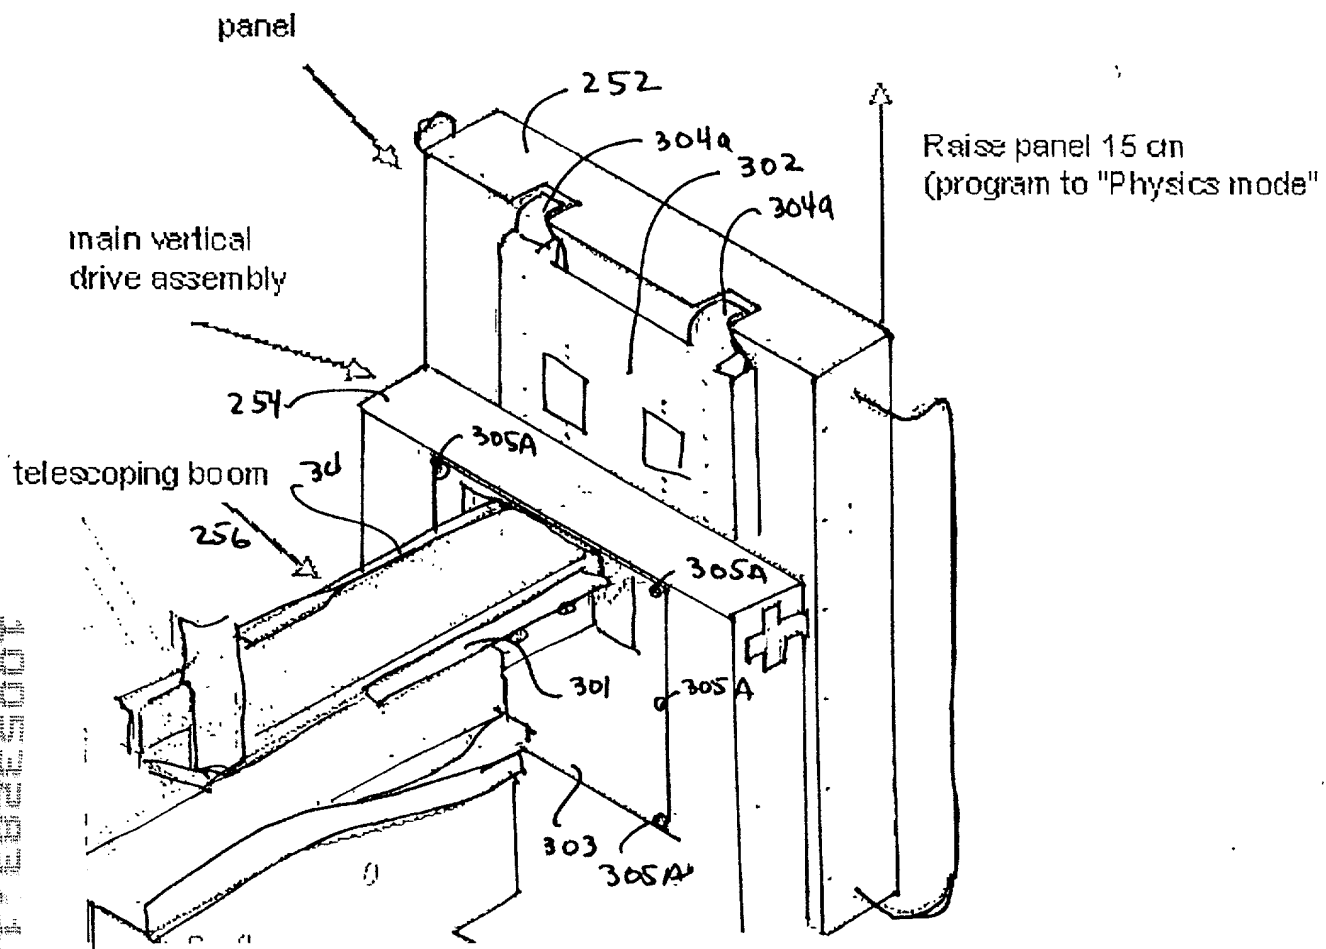


FIG. 4

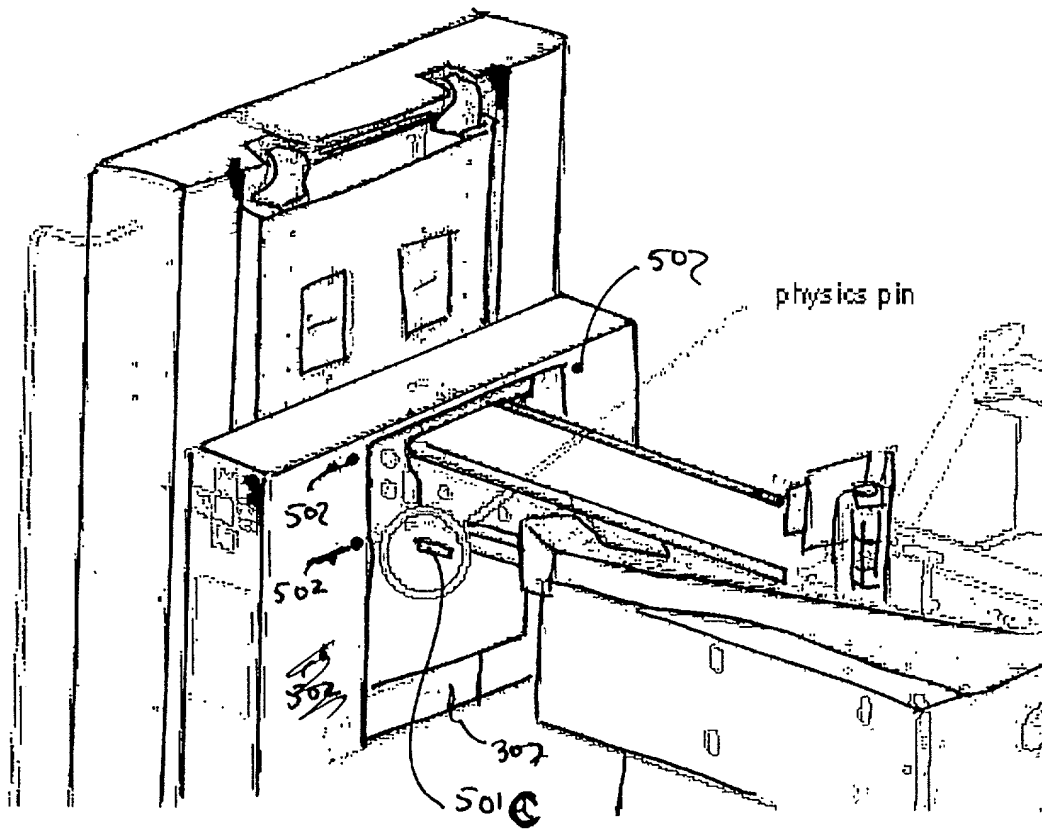


FIG. 5

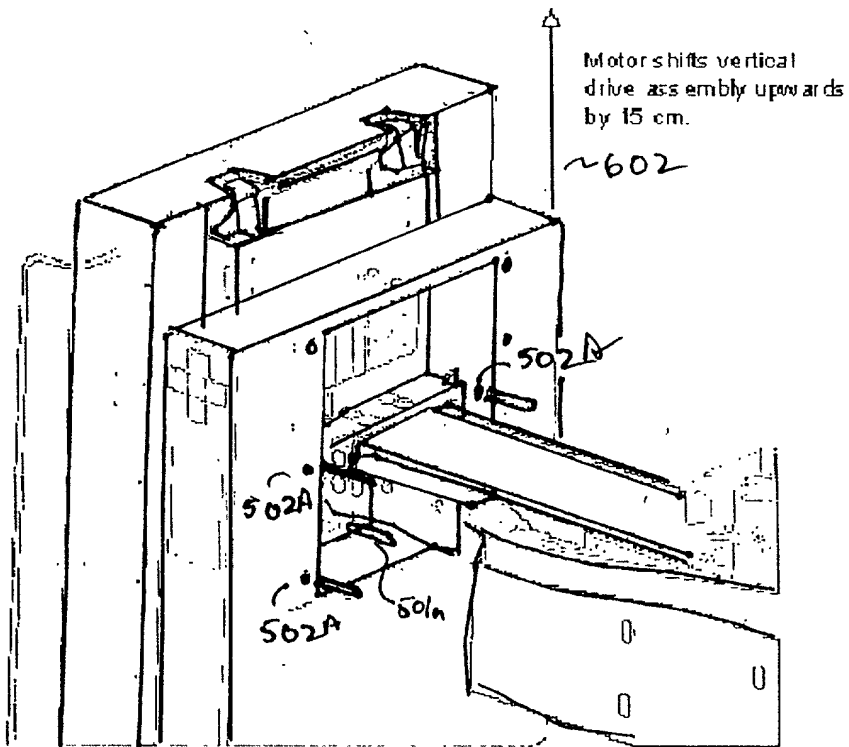


FIG. 6

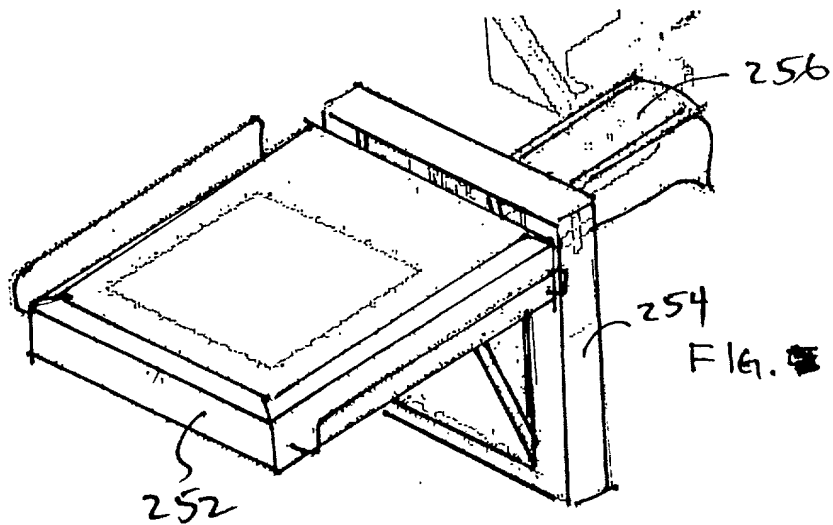


FIG. 7

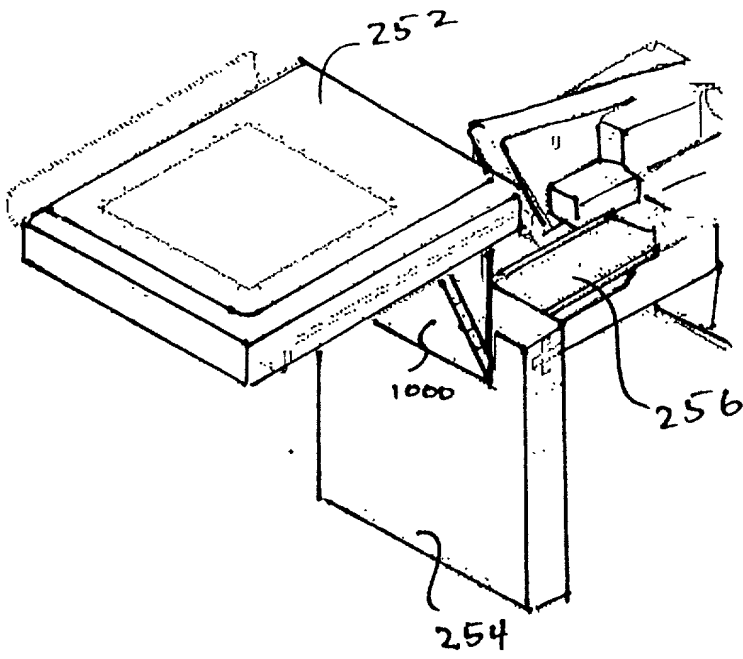


FIG. 8

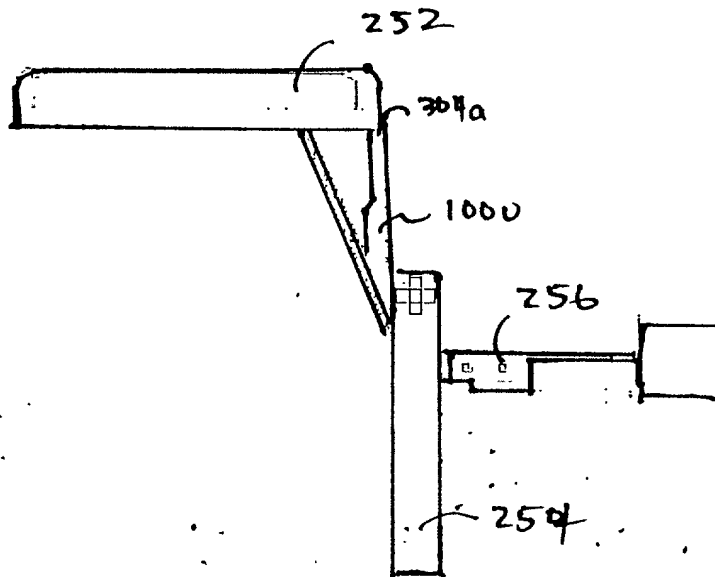


FIG. 9